

Counterlab Rx 2™ Assembly / DPD Method

Instr. #5240

1. Remove lab (#9014), all reagents, and all parts from boxes and plastic bags.
2. Set lab on flat, level surface near electrical outlet.
3. Thread correct AC Power Adapter (#6089) through interior then through hole in front of back wall of lab and connect to Gepe Slim Lite™ (#9199). Place Slim Lite inside brackets as shown below.
4. Thread correct AC Power Adapter (#6525) through interior then through hole in middle of lab and connect to SpeedStir® magnetic stirrer (#9280). Place SpeedStir between pins.

Important: AC power adapters are not interchangeable.


5. Place reagents (R-0001 to R-0012) in openings according to labels:

Top left	R-0001, R-0002, R-0003	Top right	R-0007, R-0008, R-0009
Bottom left	R-0004, R-0005, R-0006	Bottom right	R-0010, R-0011L, R-0012

6. Screw 28 mm dispenser cap (#2280) on R-0013 and R-0833.
7. Place R-0013 and R-0833 into large openings at sides of lab.
8. Place CYA cylinder (#4088) on center shelf between reagent holders as shown.
9. Place metal comparator adapter (#6582) over SpeedStir and place comparator (#9056) on adapter.
10. Place 25 mL sample tube (#9198) alongside SpeedStir and place stirring bar (#6101) in sample tube.
11. Place SampleSizer® measuring tools (#6190 and #6191) on center shelf between reagent holders as shown.
12. Place *Pool & Spa Water Chemistry* booklet (#2004B) and *Watergram®* Water Balance Calculator (#6026) inside lab.
13. Plug Slim Lite and SpeedStir AC power adapter cords into outlet.

Important: Turn off Slim Lite and SpeedStir when not in use.

Cleaning: Wipe up fresh spills with damp cloth. Clean lab periodically with a mild soap and water solution.

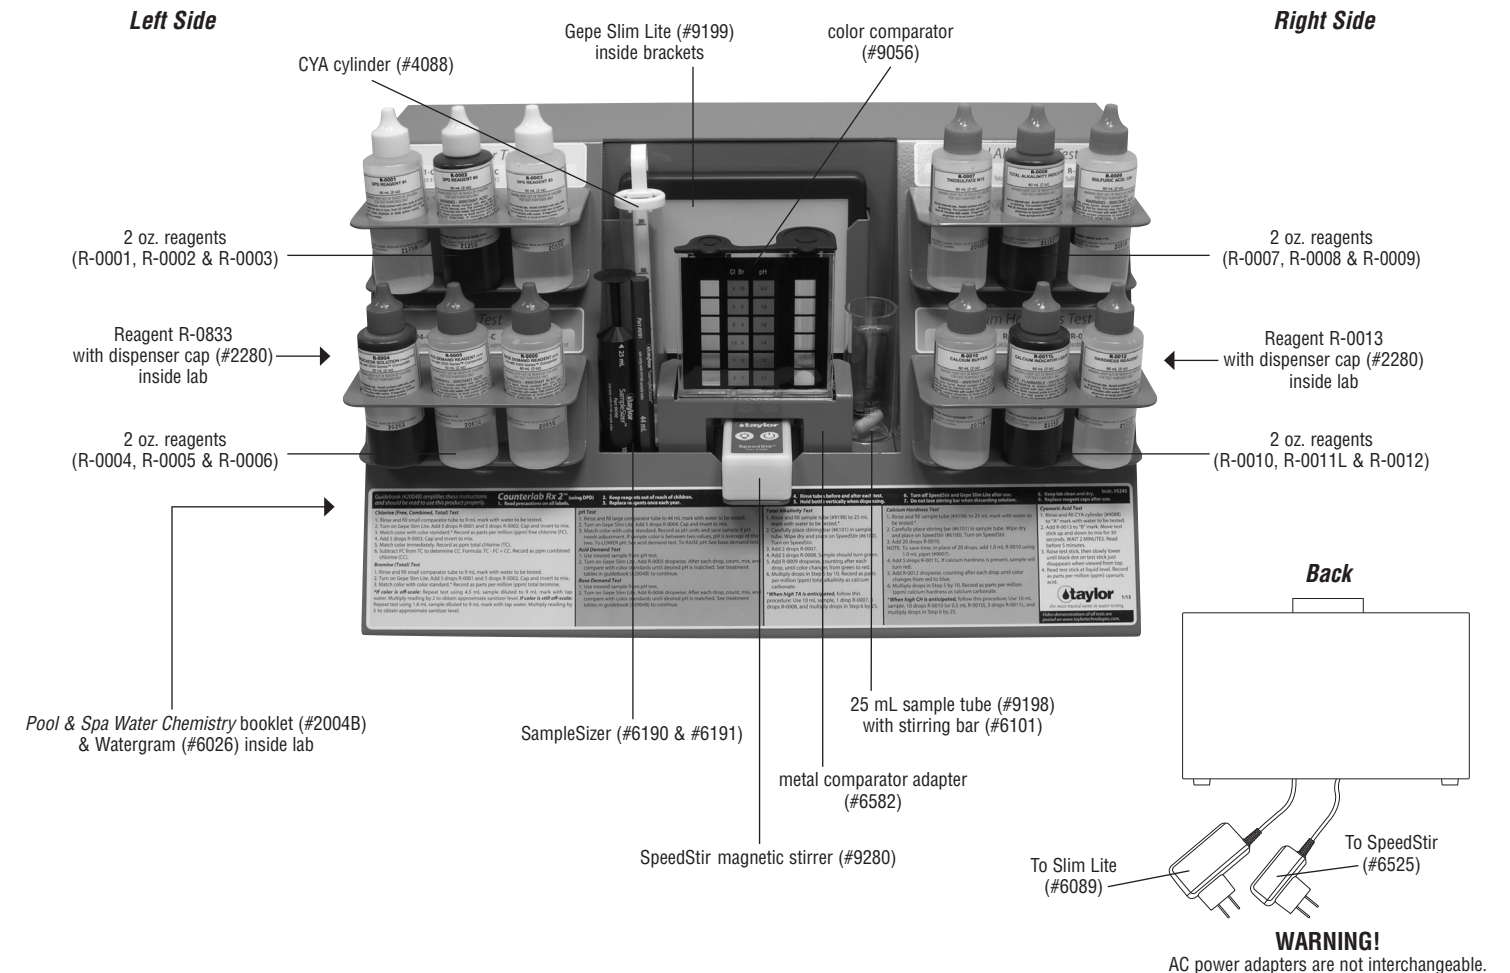

WARNING!
AC power adapters are not interchangeable.